

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXD-0001
Location: GLEN ROCK POLICE
Calibration File No.: 00588 Calib. Date: 01/06/2017 Calib. No.: 00028
Certification File No.: 00589 Cert. Date: 01/06/2017 Cert. No.: 00022
Linearity File No.: 00590 Lin. Date: 01/06/2017 Lin. No.: 00022
Solution File No.: 00604 Soln. Date: 03/18/2017 Soln. No.: 00134
Sequential File No.: 00604 File Date: 03/18/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDZJ-0091
Control Solution %: 0.100% Expires: 07/06/2018
Solution Control Lot: 16150 Bottle No.: 0897

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:20S		
Control 1 EC	0.100%	08:21S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:22S		
Control 2 EC	0.099%	08:22S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:23S		
Control 3 EC	0.099%	08:24S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:24S		

All tests within acceptable tolerance.

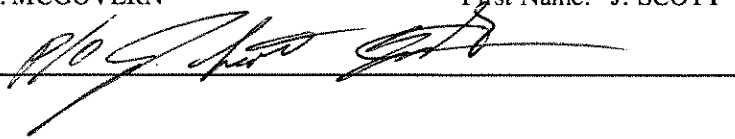
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCGOVERN

First Name: J. SCOTT

MI: -

Signature: 

Badge No.: 8130

Date: 03/18/2017