

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: GLEN ROCK POLICE

Serial No.: ARXD-0001

Calibration File No.: 00643
Certification File No.: 00629
Linearity File No.: 00630
Solution File No.: 00641
Sequential File No.: 00643

Calib. Date: 02/05/2018
Cert. Date: 10/17/2017
Lin. Date: 10/17/2017
Soln. Date: 01/23/2018
File Date: 02/05/2018

Calib. No.: 00032
Cert. No.: 00025
Lin. No.: 00025
Soln. No.: 00144

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16270

Model No.: CU-34

Serial No.: DDZJ-0090
Expires: 10/10/2018
Bottle No.: 1011

Coordinator

Last Name: KOZIEL

First Name: BARTLOMIEJ

MI:

Signature: _____


T. J. B. Koziel # 7041

Badge No.: 7041

Date: 02/05/2018

*Black Key Temperature Probe Serial.....# DDUT P2-003 (BK)

*Digital NIST Temperature Measuring System Serial.....# 170297888 (BK)

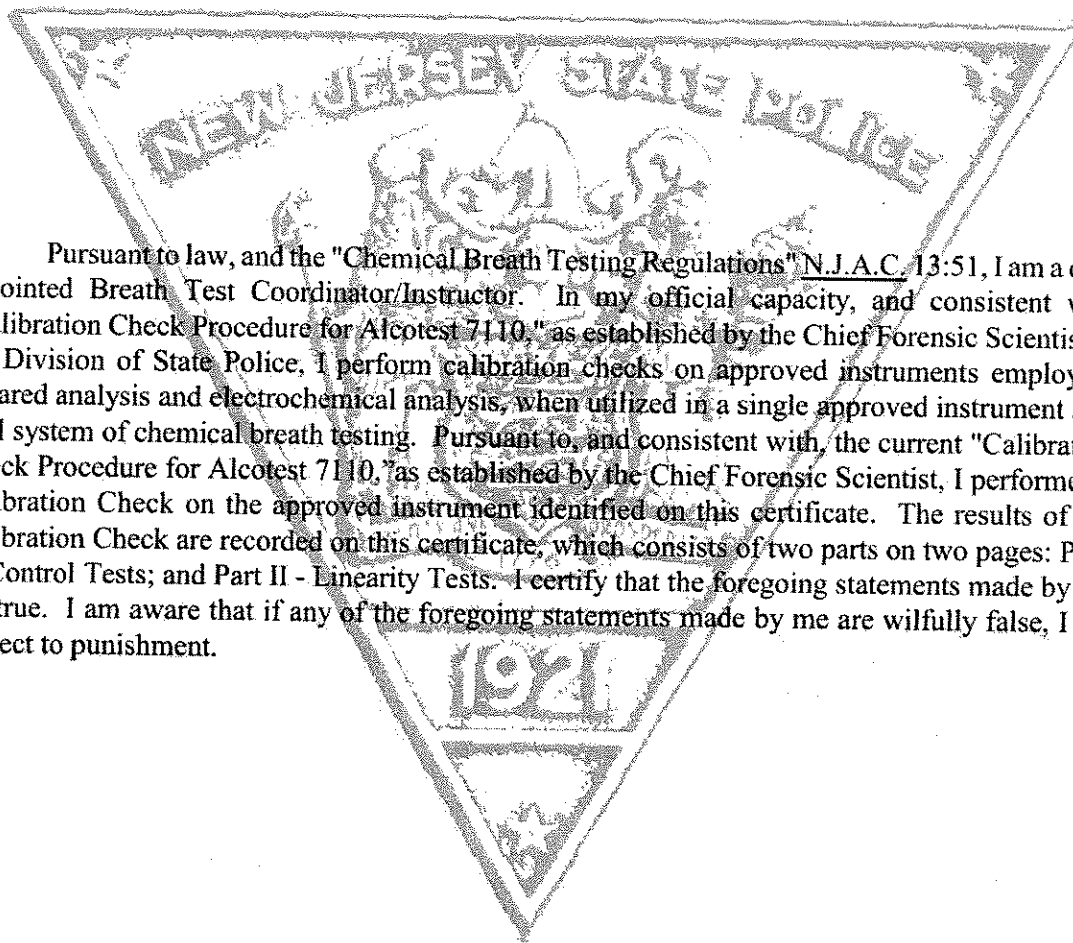

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: GLEN ROCK POLICE
Serial No.: ARXD-0001
Calibration File No.: 00643
Certification File No.: 00644
Linearity File No.: 00630
Solution File No.: 00641
Sequential File No.: 00644
Calib. Date: 02/05/2018
Cert. Date: 02/05/2018
Lin. Date: 10/17/2017
Soln. Date: 01/23/2018
File Date: 02/05/2018
Calib. No.: 00032
Cert. No.: 00026
Lin. No.: 00025
Soln. No.: 00144

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16270
Model No.: CU-34
Serial No.: DDZJ-0090
Expires: 10/10/2018
Bottle No.: 1011

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 14:22S | | |
| Control 1 EC | 0.100% | 14:23S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 14:23S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:24S | | |
| Control 2 EC | 0.100% | 14:24S | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 14:24S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:25S | | |
| Control 3 EC | 0.098% | 14:26S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 14:26S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:27S | | |

All tests within acceptable tolerance.

Coordinator

Last Name: KOZIEL

First Name: BARTLOMIEJ

MI:

Signature: T. I. B. Koziel # 7041

Badge No.: 7041

Date: 02/05/2018

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXD-0001 |
| Location: | GLEN ROCK POLICE | |
| Calibration File No.: | 00643 | Calib. Date: 02/05/2018 |
| Certification File No.: | 00644 | Calib. No.: 00032 |
| Linearity File No.: | 00645 | Cert. Date: 02/05/2018 |
| Solution File No.: | 00641 | Cert. No.: 00026 |
| Sequential File No.: | 00645 | Lin. Date: 02/05/2018 |
| | | Lin. No.: 00026 |
| | | Soln. Date: 01/23/2018 |
| | | Soln. No.: 00144 |
| | | File Date: 02/05/2018 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.040% | Serial No.: DDWE S3-0196 |
| Solution Control Lot: | 16230 | Expires: 09/19/2018 |
| | | Bottle No.: 0721 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.080% | Serial No.: DDWE S3-0205 |
| Solution Control Lot: | 16250 | Expires: 09/27/2018 |
| | | Bottle No.: 0010 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.160% | Serial No.: DDRF S3-0011 |
| Solution Control Lot: | 16260 | Expires: 10/03/2018 |
| | | Bottle No.: 0728 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 14:36S | | |
| Control 1 EC | 0.043% | 14:36S | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.040% | 14:36S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:38S | | |
| Control 2 EC | 0.042% | 14:38S | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.039% | 14:38S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:40S | | |
| Control 3 EC | 0.082% | 14:40S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.080% | 14:40S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:42S | | |
| Control 4 EC | 0.083% | 14:43S | 34.0°C | *** TEST PASSED *** |
| Control 4 IR | 0.080% | 14:43S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:44S | | |
| Control 5 EC | 0.165% | 14:45S | 33.9°C | *** TEST PASSED *** |
| Control 5 IR | 0.163% | 14:45S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:46S | | |
| Control 6 EC | 0.164% | 14:47S | 34.0°C | *** TEST PASSED *** |
| Control 6 IR | 0.162% | 14:47S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:49S | | |

All tests within acceptable tolerance.

Coordinator

Last Name: KOZIEL

First Name: BARTLOMIEJ

MI:

Signature: _____

T. J. B. Koziel # 7041

Badge No.: 7041

Date: 02/05/2018

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|-------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXD-0001 |
| Location: | GLEN ROCK POLICE | |
| Calibration File No.: | 00643 | Calib. Date: 02/05/2018 |
| Certification File No.: | 00644 | Cert. No.: 00032 |
| Linearity File No.: | 00645 | Cert. Date: 02/05/2018 |
| Solution File No.: | 00646 | Lin. No.: 00026 |
| Sequential File No.: | 00646 | Soln. No.: 00145 |
| | | File Date: 02/05/2018 |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDZJ-0090 |
| Solution Control Lot: | 17110 | Expires: 03/20/2019 |
| | | Bottle No.: 0489 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 15:54S | | |
| Control 1 EC | 0.103% | 15:55S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.102% | 15:55S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:55S | | |
| Control 2 EC | 0.101% | 15:56S | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.102% | 15:56S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:57S | | |
| Control 3 EC | 0.101% | 15:57S | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.102% | 15:57S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:58S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUN P2-368 (BK)

Changed By:

Last Name: KOZIEL

First Name: BARTLOMIEJ

MI:

Signature: *T. J. B. Koziel # 7041*

Badge No.: 7041

Date: 02/05/2018

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

7-27-15

SERIAL NUMBER:

ARXD-0001

Dräger Safety Diagnostics, Inc.

BC



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-8483336

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 170297888 Manufacturer: Control Company

Standards/Equipment:

| Description | Serial Number | Due Date | NIST Traceable Reference |
|-------------------------------------|---------------|----------|--------------------------|
| Temperature Calibration Bath TC-231 | A79341 | | |
| Thermistor Module | A27129 | 12/01/17 | 1000401760 |
| Temperature Probe | 5267 | 12/06/17 | B6B30059 |
| Temperature Calibration Bath TC-191 | A42238 | | |
| Thermistor Module | A27129 | 12/01/17 | 1000401760 |
| Temperature Probe | 5202 | 12/19/17 | B6B30058-1 |
| Temperature Calibration Bath TC-218 | A73332 | | |
| Thermistor Probe | 5356 | 1/10/18 | B7104024 |
| Readout, Digital Thermometer | B5C344 | 3/12/18 | B7314035 |
| Temperature Calibration Bath TC-275 | B16388 | | |
| Thermistor Probe | 5357 | 1/06/18 | B7104023 |
| Readout, Digital Thermometer | B5C344 | 3/12/18 | B7314035 |

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 4/22/17 Due Date: 4/22/19
Test Conditions: 23.9°C 61.0 %RH 1012 mBar

Calibration Data: (New Instrument)

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min | Max | ±U | TUR |
|---------|---------|----------|--------|---------|---------|--------|--------|---------|-------|------|
| °C | | N.A. | | 0.002 | -0.001 | Y | -0.048 | 0.052 | 0.010 | >4:1 |
| °C | | N.A. | | 25.000 | 24.999 | Y | 24.950 | 25.050 | 0.010 | >4:1 |
| °C | | N.A. | | 49.998 | 50.000 | Y | 49.948 | 50.048 | 0.010 | >4:1 |
| °C | | N.A. | | 99.998 | 100.003 | Y | 99.948 | 100.048 | 0.010 | >4:1 |

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2008-AQ-HOU-RVA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0196

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0205

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

Other: _____

Serial Number:

DDRES3-0011

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDUSP2-003

Certification Date:

9-8-17

Next Certification Due:

9-8-18

Probe Value:

98

Dräger, Inc.

BC



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: **ALCOTEST® CU34**

Model: **MARK IIA**

Other: _____

Serial Number:

DDZJ-0090

Certification Date

6-12-17

Technician

72

Re-Certification Due Date

6-12-18

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accurate verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDUNP2-368

Certification date:

6-12-17

Next Certification due:

6-12-18

Probe Value

102

Dräger Safety Diagnostics, Inc.
Technical Service Department

72



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/19/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 10, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of October, 2016.

[Signature]
Notary
JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/27/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0492 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 19, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of September, 2016.

[Signature]
Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/04/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0965 to 0.0975 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 27, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2016.

[Signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

CHRISTOPHER S. PORRINO
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/13/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1928 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaoui]

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 17 day of October, 2016.

Notary
JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 03/29/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17110

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1231 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 20, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30th day of March, 2017.

Mary E. McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
 This is to certify that

Bartlomiej P. Koziel
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Aicofest 7110 MEM-C

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF July

IN THE YEAR AND ELEVEN


 SUPERINTENDENT
 NEW JERSEY STATE POLICE


 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------------|---------------------------|------------|
| 1. 7-15-13 | M.L.P.A | R. J. |
| 2. 9-16-15 | BERLEN C.P.A | C.S. |
| 3. 9-12-17 | BERLEN C.P.A | C.S. |
| 4. | | |
| 5. | | |
| 6. | | |
| 7. | | |
| 8. | | |
| 9. | | |

8.P 2335 (Rev. 03/10)

DEPARTMENT OF
Law and Public Safety
 This is to certify that

Bartłomiej Koziel
 Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 141 OF
 THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS **16th** DAY OF **December**

THIRTHOUSAND AND **Sixteen**

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES:

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------|------------------------|------------|
| 1. | | |
| 2. | | |
| 3. | | |
| 4. | | |
| 5. | | |
| 6. | | |
| 7. | | |
| 8. | | |
| 9. | | |

S.P. 292B (Rev. 07/16)