

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXD-0001
Location:	GLEN ROCK POLICE		
Calibration File No.:	00670	Calib. Date:	05/31/2018
Certification File No.:	00671	Cert. No.:	00033
Linearity File No.:	00672	Cert. Date:	05/31/2018
Solution File No.:	00679	Lin. Date:	05/31/2018
Sequential File No.:	00679	Soln. Date:	10/09/2018
		File Date:	10/09/2018
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDZJ-0091
Solution Control Lot:	18090	Expires:	03/13/2020
		Bottle No.:	0746

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:02D		
Control 1 EC	0.099%	18:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:03D		
Control 2 EC	0.098%	18:04D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:04D		
Control 3 EC	0.099%	18:05D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MCGOVERN

First Name: J. SCOTT

MI: -

Signature: \_\_\_\_\_

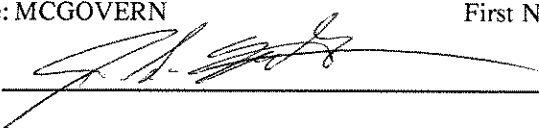

Badge No.: 8130

Date: 10/09/2018